

**Centers for Disease Control and Prevention
Model Performance Evaluation Program
Human Immunodeficiency Virus Type 1 (HIV-1)
Testing for p24 Antigen**

**Figures Used for the Analysis
of the June 29, 1998 Performance Evaluation
Testing Results Reported by Participant Laboratories**

**U.S. DEPARTMENT OF HEALTH AND HUMAN SERVICES
Public Health Service
Centers for Disease Control and Prevention
Public Health Practice Program Office
Division of Laboratory Systems
Atlanta, Georgia 30333**

**Use of trade names is for identification only and does not constitute endorsement by the
Public Health Service or by the
U.S. Department of Health and Human Services.**

Report of the June 29, 1998 Human Immunodeficiency Virus Type I (HIV-1) p24 Antigen Performance Evaluation Sample Testing Results Provided by Participant Laboratories in the Model Performance Evaluation Program, Centers for Disease Control and Prevention (CDC).

The production of this report was coordinated in CDC by:

Public Health Practice Program Office.....Edward L. Baker, M.D., M.P.H., Director
Division of Laboratory Systems.....Carlyn L. Collins, M.D., M.P.H., Director
Laboratory Practice Assessment Branch.....Thomas L. Hearn, Ph.D., Chief

The material in this report was developed and prepared by:

Model Performance Evaluation Program (MPEP).....William O. Schalla, M.S., Chief
MPEP HIV-1 Performance Evaluation.....Sharon O. Blumer, M.S.,
HIV-1 Project Coordinator

Information about this report should be addressed to the Model Performance Evaluation Program by calling (770) 488-8090 or (770) 488-8098.

**SUPPLEMENTAL INFORMATION FOR COMPREHENDING
THE NUMBERS USED TO LABEL FIGURES
IN THIS REPORT**

The "N=" that appears on each graph represents the number of laboratories that reported results. For some graphs, laboratories reported results using more than one test kit for a specific test type; therefore, the AN=@ may exceed the actual number of laboratories participating in the survey. In figures 1-3 and 5-6, the vertical axis is labeled either as frequency of results or percentage of reporting laboratories; in figure 4, the horizontal axis is labeled as percentage of reporting laboratories. In all figures, the number appearing directly above each bar represents a frequency of results only.

**Centers for Disease Control and Prevention (CDC)
Model Performance Evaluation Program for
Human Immunodeficiency Virus Type I (HIV-1) p24 Antigen Testing**

**Table 1. CDC HIV-1 p24 Antigen Testing Results for the June 29, 1998
Participant Laboratory Panel Samples**

Panel Letter Interpretation ²	Vial Label	CDC Donor Number	CDC Test Results ¹	Test Kit Manufacturer	CDC
A	A1, A4	01	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAb ³ Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
	A2	03	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative
	A3	02	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
	A5	04	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative
	B	B1	04	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen
B2, B5		01	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
B3		03	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative
B4		02	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
C	C1, C3	01	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
	C2	04	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative
	C4	03	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative
	C5	02	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
D	D1	02	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
	D2, D4	01	p24 Antigen detected p24 Antigen detected p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Positive Positive Positive
	D3	04	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative
	D5	03	No p24 Antigen detected No p24 Antigen detected No p24 Antigen detected	Abbott HIVAG-1 MAB Coulter HIV-1 p24 Antigen Organon HIV-1 Antigen	Negative Negative Negative

¹ Result based on testing performed in two separate laboratories.

² The CDC interpretation is consistent with the manufacturer's criteria for interpretation of results.
Positive = Presence of HIV-1 p24 antigen confirmed; Negative = p24 antigen not detected

³ **MAb = monoclonal antibody**

Figure 1. Frequency of HIV-1 p24 Antigen Test Result Interpretations, by Sample Type (Reactivity), for Qualitative and Neutralization Tests Reported by Participant Laboratories for the June 29, 1998 Shipment

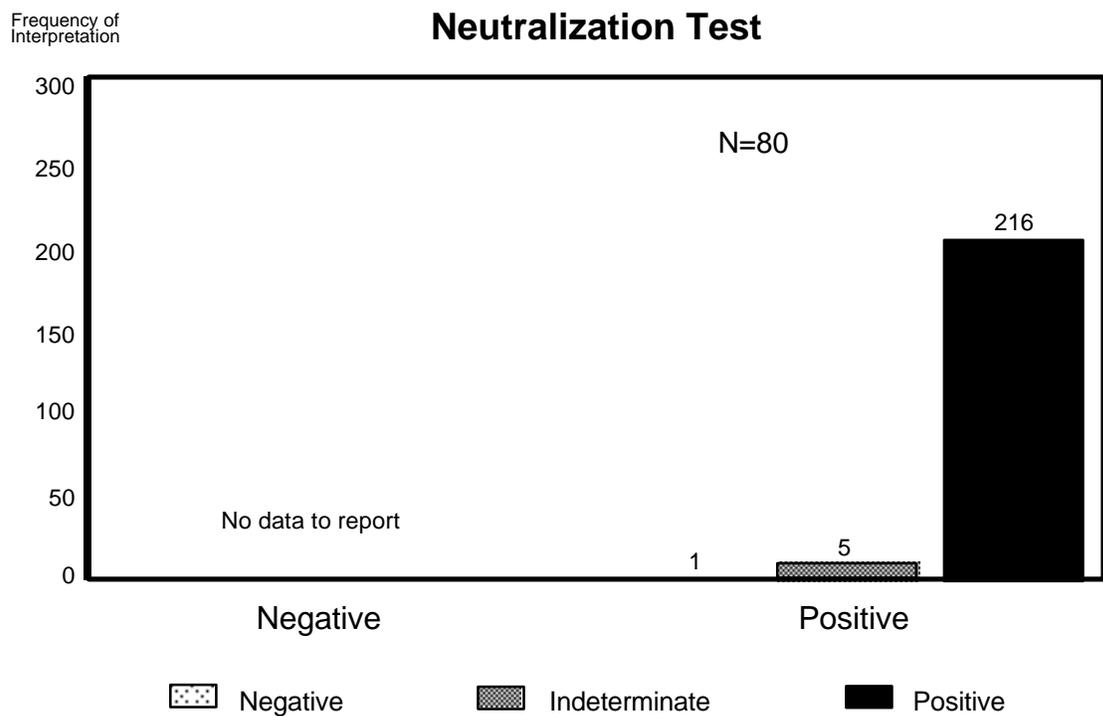
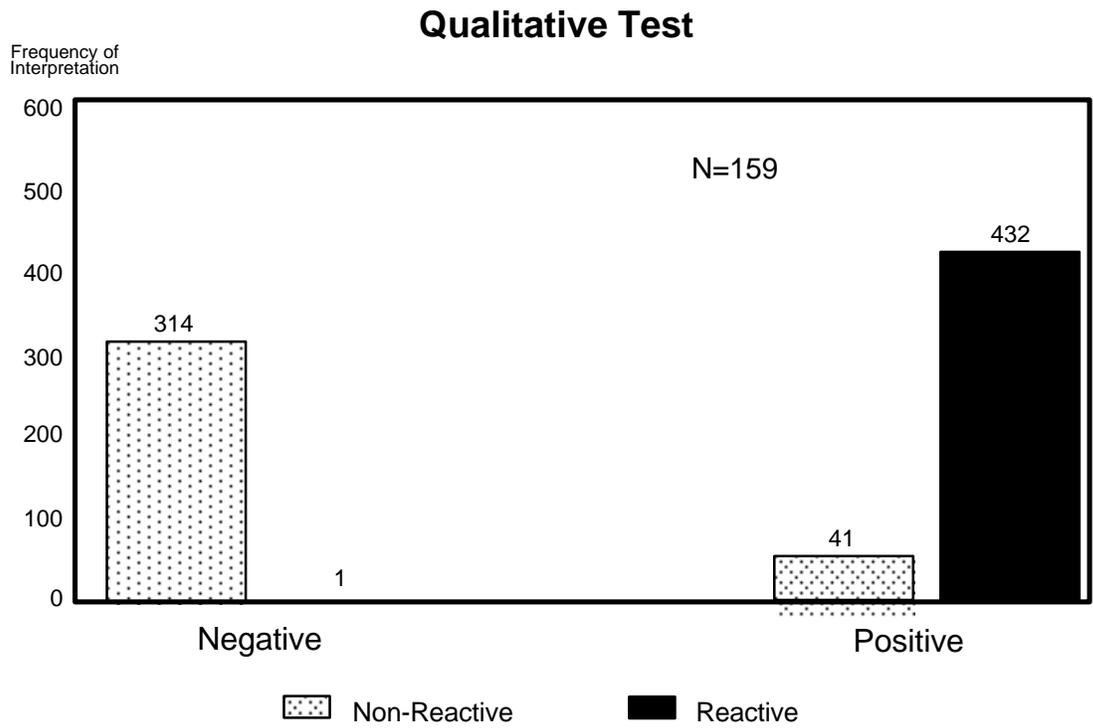


Figure 2. Percentage of Participant Laboratories, by Laboratory Type, that Reported HIV-1 p24 Antigen Qualitative, Neutralization, and Quantitative Results to the CDC for the June 29, 1998 Shipment

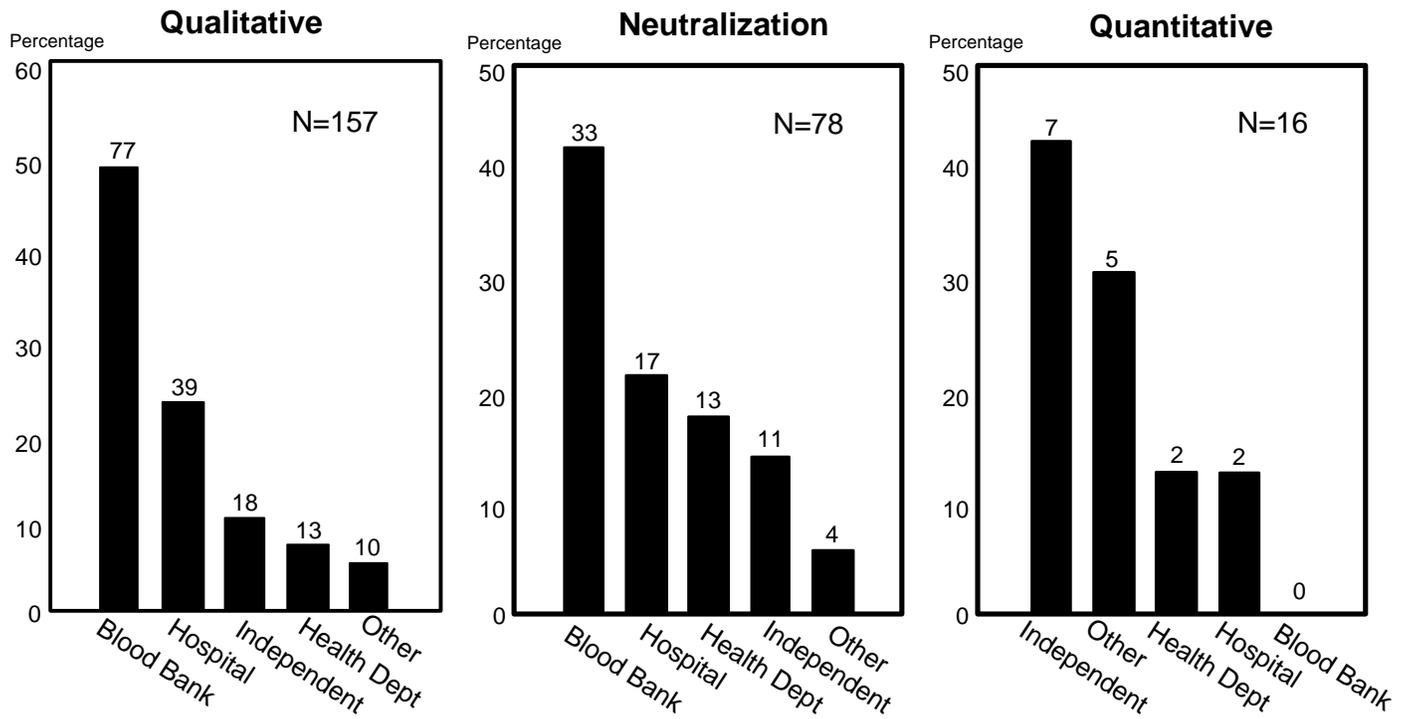


Figure 3. Combination of HIV-1 p24 Antigen Tests Reported by Participant Laboratories for the June 29, 1998 Shipment




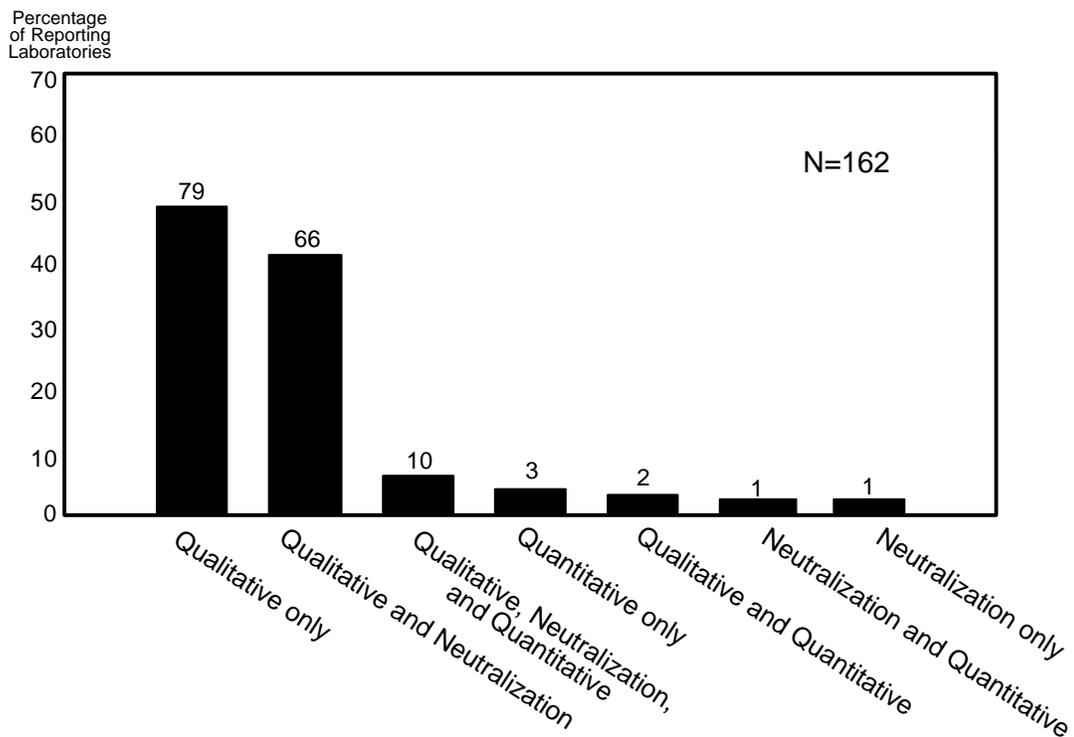


Figure 4. Types of Test Kits Used for HIV-1 p24 Antigen Qualitative, Neutralization, and Quantitative Tests Reported to CDC by Participant Laboratories in the June 29, 1998 Shipment

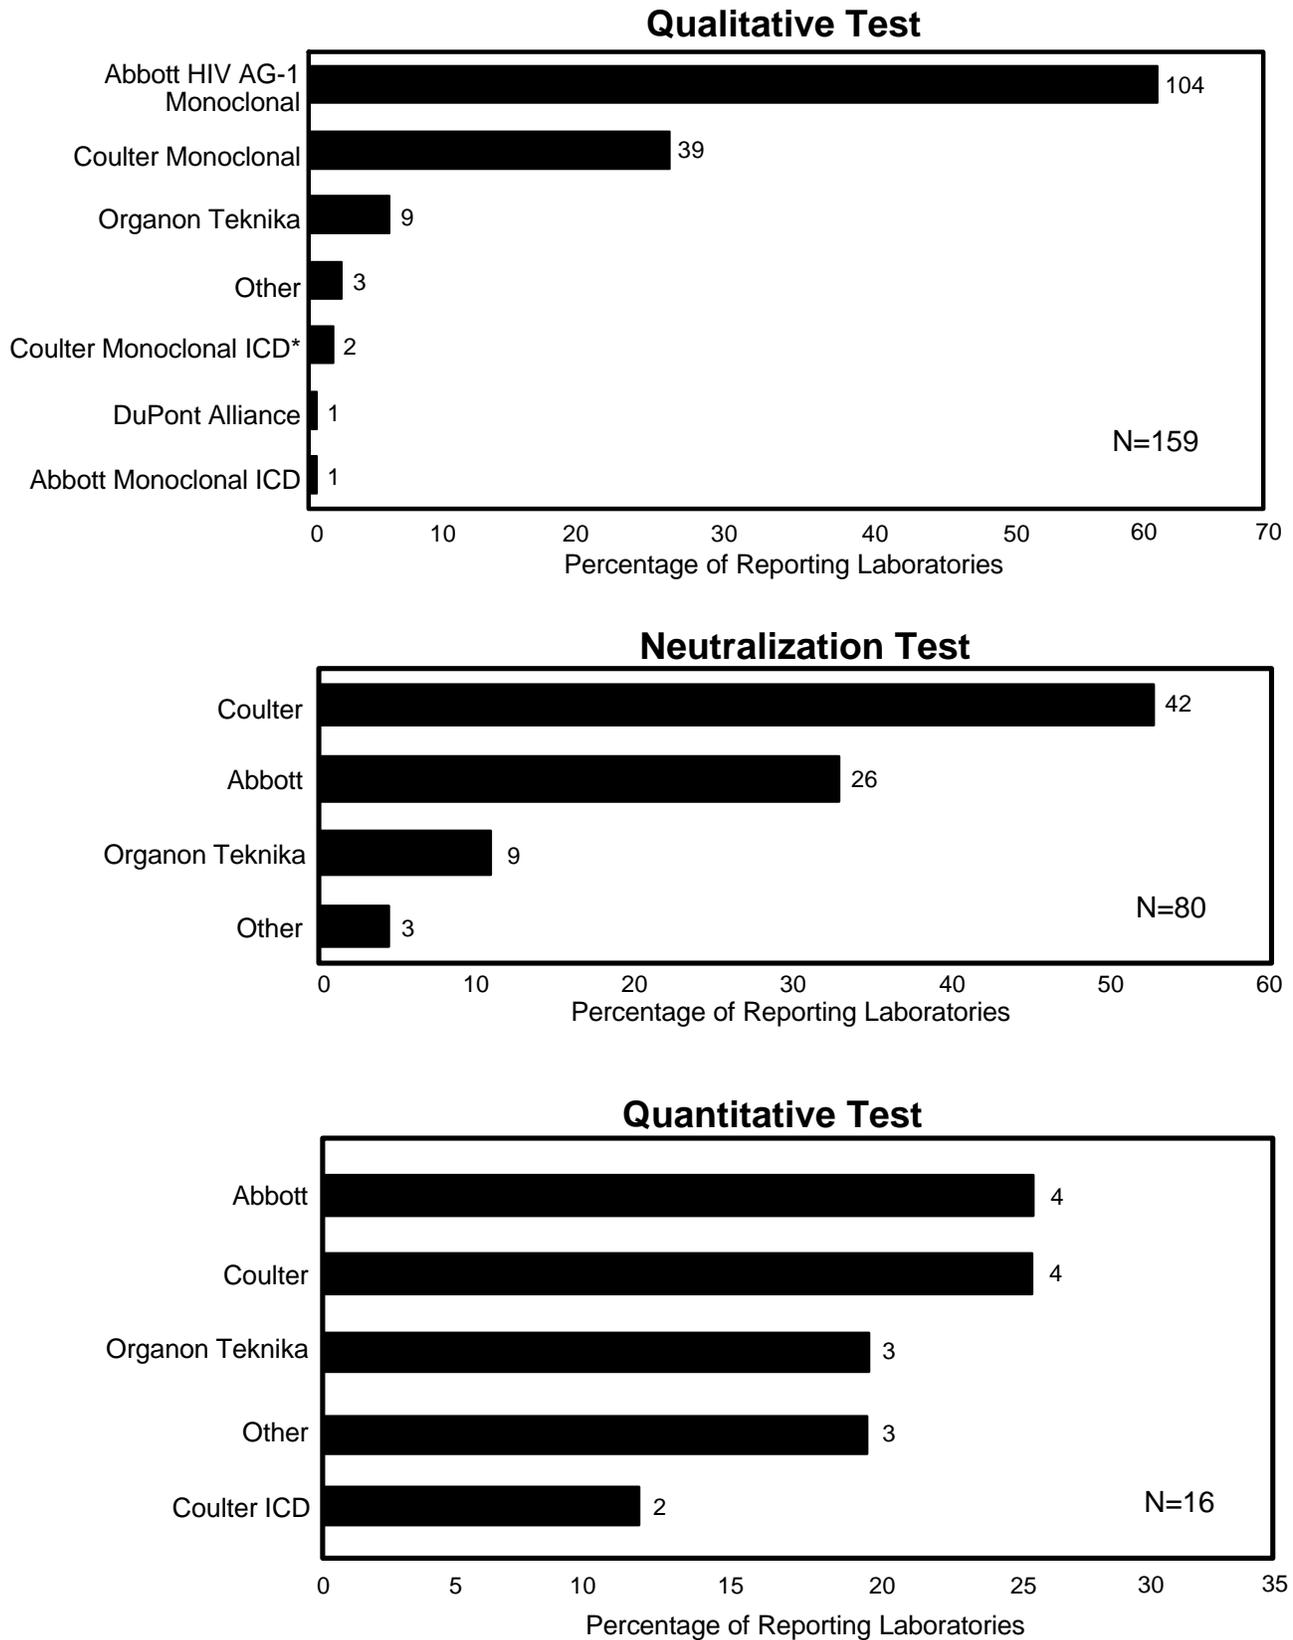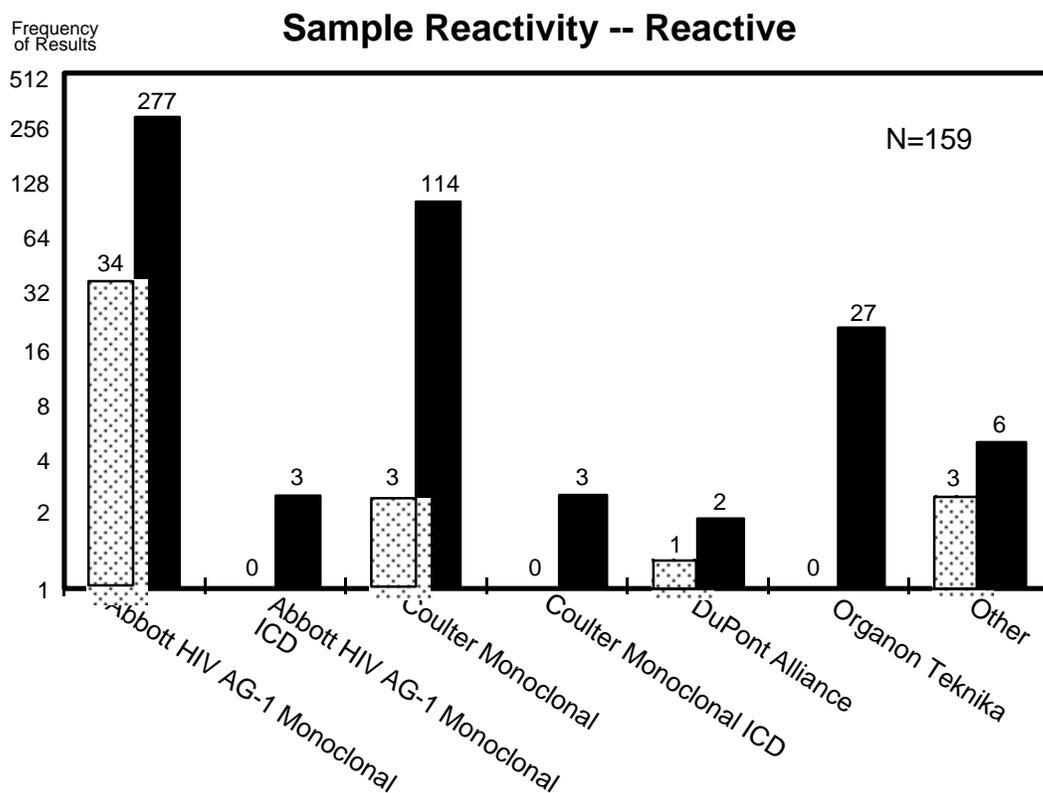

*ICD=Immune Complex Dissociation

Figure 5. HIV-1 p24 Antigen Qualitative Test Results, by Kit Manufacturer, Reported by Participant Laboratories for the June 29, 1998 Shipment

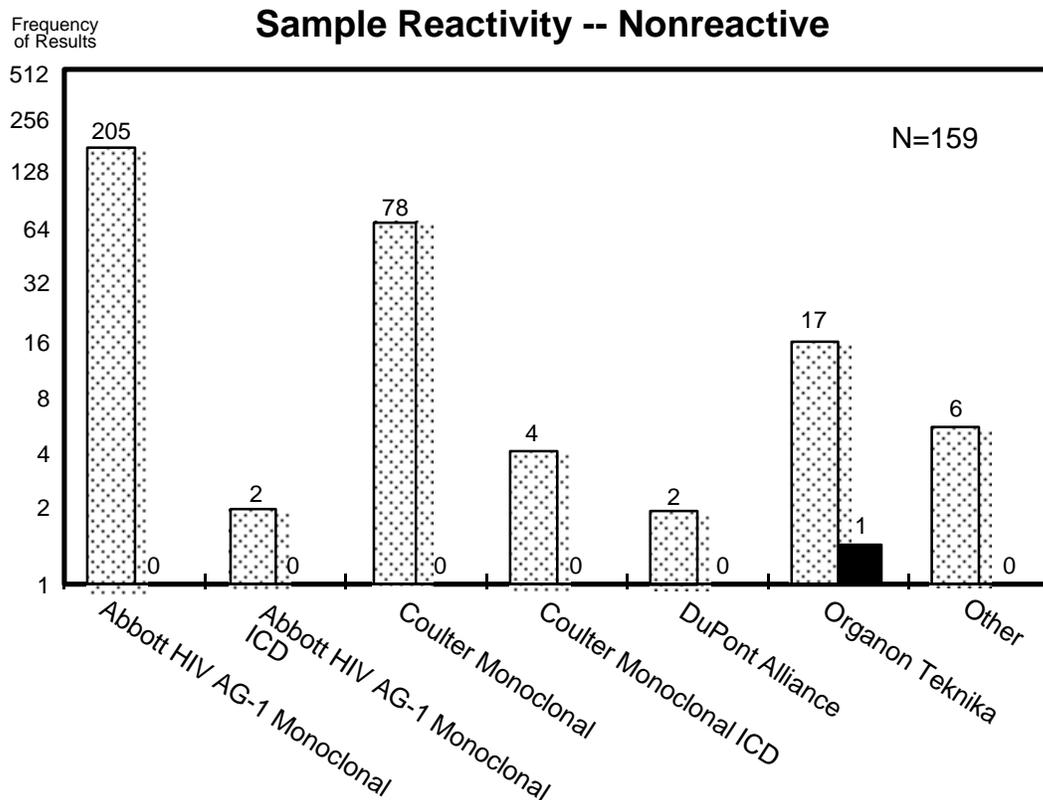

Nonreactive
 Reactive

Figure 6. HIV-1 p24 Antigen Neutralization Test Results, by Kit Manufacturer, Reported by Participant Laboratories for the June 29, 1998 Shipment

Sample Reactivity -- Negative

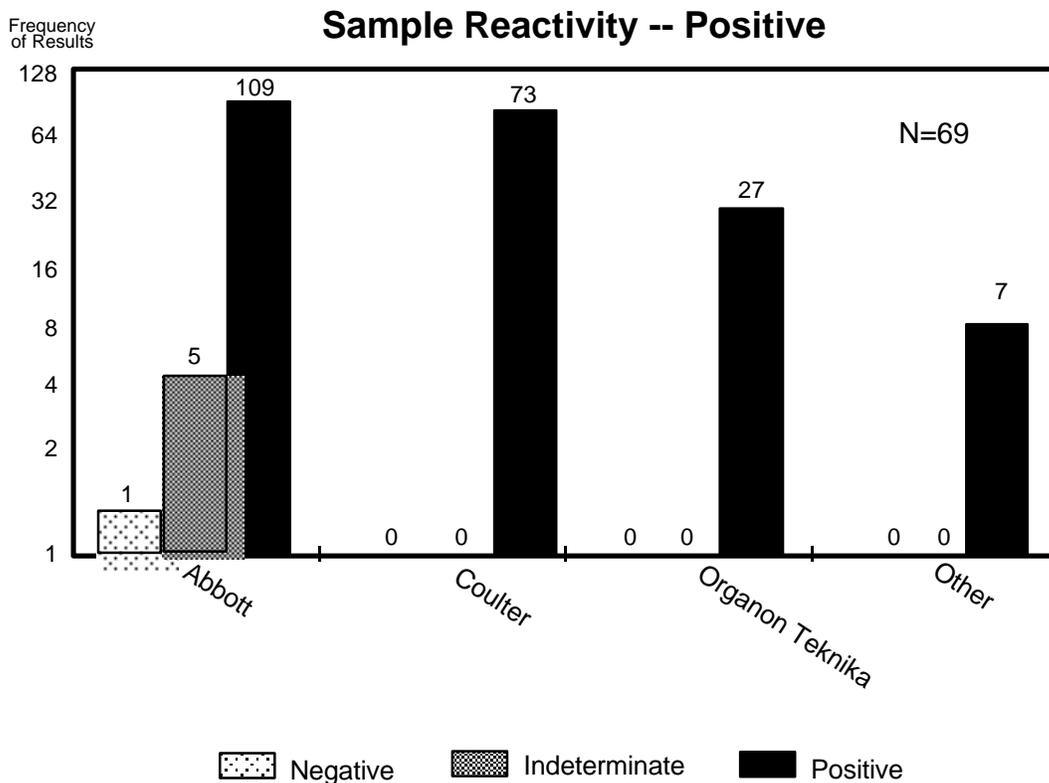
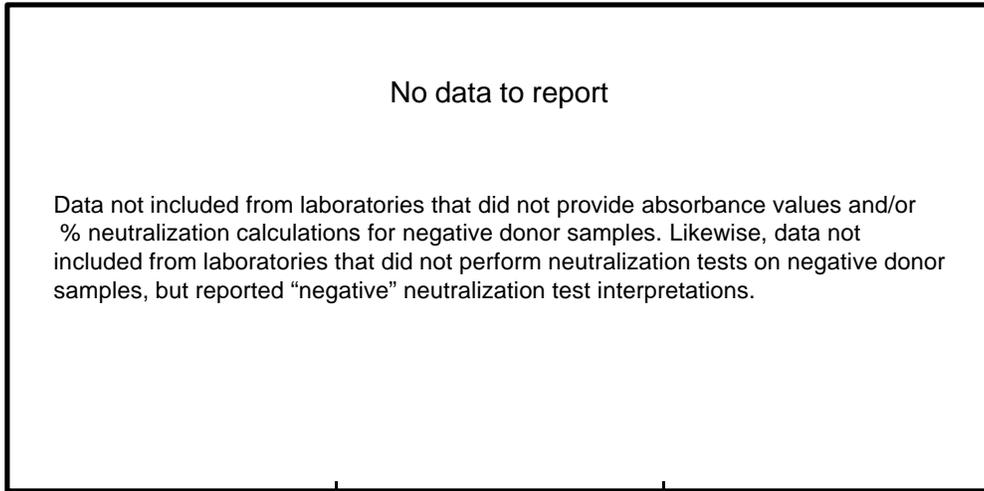


Table 2. Results of the HIV-1 p24 Antigen Neutralization Test Reported by Participant Laboratories for the June 29, 1998 Performance Evaluation Shipment

CDC Donor #1
Donor Status: HIV-1 Infected
Panel Vial Labels: A1, B2, C1, D2

Test Kit	No. of Results Confirming p24	No. of Results Not Confirming p24	Range of Results Reported % Neutralization		
			minimum	median	maximum
Abbott	42	0	71.0	89.1	120.8
Coulter	25	0	61.9	79.8	99.5
Organon Teknika	9	0	79.5	87.0	91.9
Other	3	0	98.8	99.0	100.0

CDC Donor #1 - Duplicate
Donor Status: HIV-1 Infected
Panel Vial Labels: A4, B5, C3, D4

Test Kit	No. of Results Confirming p24	No. of Results Not Confirming p24	Range of Results Reported % Neutralization		
			minimum	median	maximum
Abbott	42	0	63.5	89.5	121.2
Coulter	25	0	58.2	75.9	101.0
Organon Teknika	9	0	83.2	89.0	93.6
Other	3	0	98.8	100.4	103.4

Table 2. Results of the HIV-1 p24 Antigen Neutralization Test Reported by Participant Laboratories for the June 29, 1998 Performance Evaluation Shipment (Continued)

CDC Donor #2
Donor Status: HIV-1 Infected
Panel Vial Labels: A3, B4, C5, D1

Test Kit	No. of Results Confirming p24	No. of Results Not Confirming p24	Range of Results Reported % Neutralization		
			minimum	median	maximum
Abbott	25	6	47.7	68.3	114.3
Coulter	23	0	51.2	76.5	97.9
Organon Teknika	9	0	82.3	89.5	92.0
Other	1	0	97.6	97.6	97.6

Table 3. Results of the HIV-1 p24 Antigen Quantitative Test Reported by Participant Laboratories for the June 29, 1998 Performance Evaluation Shipment

**CDC Donor #1
 Donor Status: HIV-1 Infected
 Panel Vial Labels: A1, B2, C1, D2**

Test Kit	No. of Results Quantitating p24	No. of Results Not Quantitating p24	Range of Results Reported Concentration (pg/ml)		
			minimum	median	maximum
Abbott	4	0	9.5	34.7	97.4
Abbott ICD	1	0	86.0	86.0	86.0
Coulter	2	0	19.4	24.2	29.0
Coulter ICD	4	0	44.0	201.0	268.5
Organon Teknika	3	0	16.2	20.2	64.9
Other	3	0	7.5	115.7	120.0

**CDC Donor #1 - Duplicate
 Donor Status: HIV-1 Infected
 Panel Vial Labels: A4, B5, C3, D4**

Test Kit	No. of Results Quantitating p24	No. of Results Not Quantitating p24	Range of Results Reported Concentration (pg/ml)		
			minimum	median	maximum
Abbott	4	0	8.6	30.6	63.1
Abbott ICD	1	0	99.5	99.5	99.5
Coulter	2	0	18.8	20.9	23.0
Coulter ICD	4	0	39.0	204.5	252.7
Organon Teknika	3	0	16.3	16.4	66.0
Other	3	0	9.2	110.0	130.0

Table 3. Results of the HIV-1 p24 Antigen Quantitative Test Reported by Participant Laboratories for the June 29, 1998 Performance Evaluation Shipment (Continued)

CDC Donor #2
 Donor Status: HIV-1 Infected
 Panel Vial Labels: A3, B4, C5, D1

Test Kit	No. of Results Quantitating p24	No. of Results Not Quantitating p24	Range of Results Reported Concentration (pg/ml)		
			minimum	median	maximum
Abbott	2	0	100.0	110.5	121.0
Abbott ICD	1	0	189.3	189.3	189.3
Coulter	2	0	9.1	15.1	21.0
Coulter ICD	3	0	24.0	673.5	785.0
Organon Teknika	3	0	13.3	21.3	66.4
Other	3	0	3.5	144.8	182.0